

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

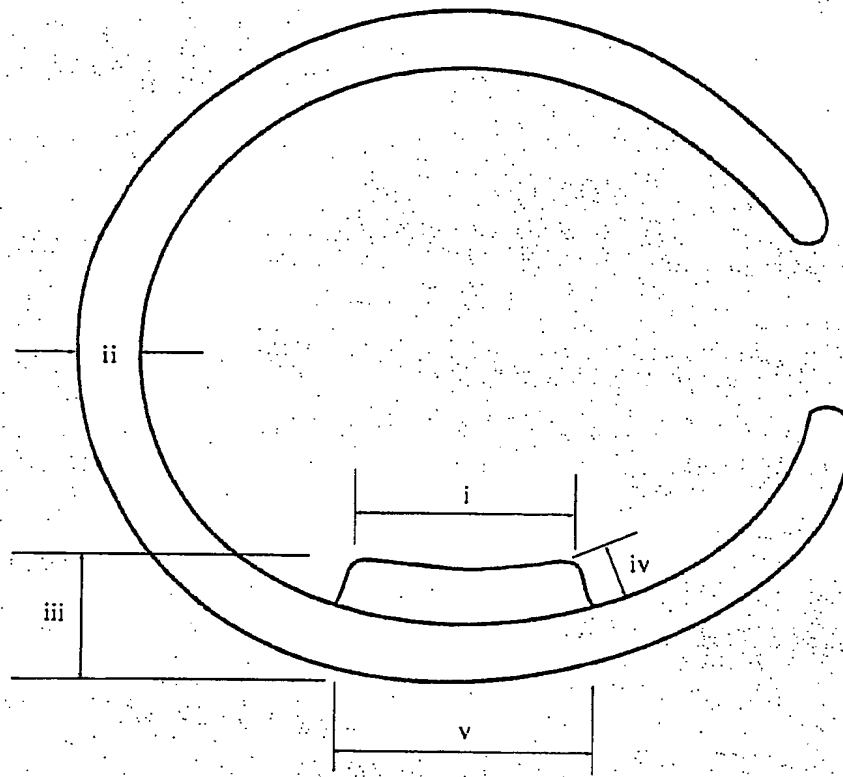


Fig. 1

Fig 1	min	max	optimum
i	6.0	10.0	8.0
ii	0.8	1.8	1.0
iii	2.0	3.8	2.8
iv	1.0	2.5	1.6
v	8.0	12.0	10.0

All measurements in millimetres



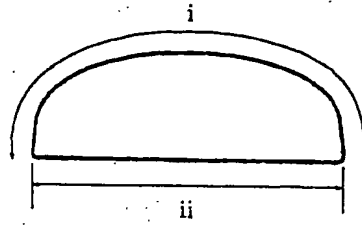


Fig. 2A

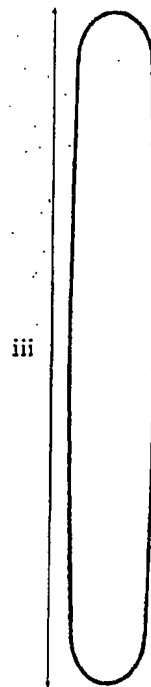


Fig. 2B

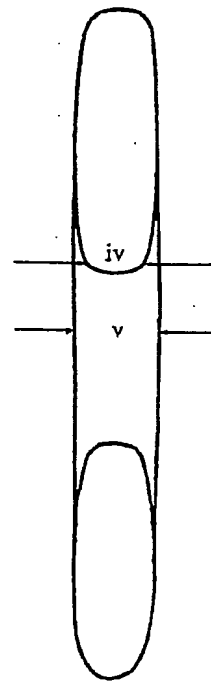


Fig. 2C

Fig 2a	min	max	optimum
i	4.9	10.0	6.5
ii	3.0	8.0	4.5
Fig 2b			
iii	18.0	26.0	22.4
Fig 2c			
iv	3.0	8.0	4.0
v	3.0	8.0	4.5

All measurements in millimetres

Technical specifications

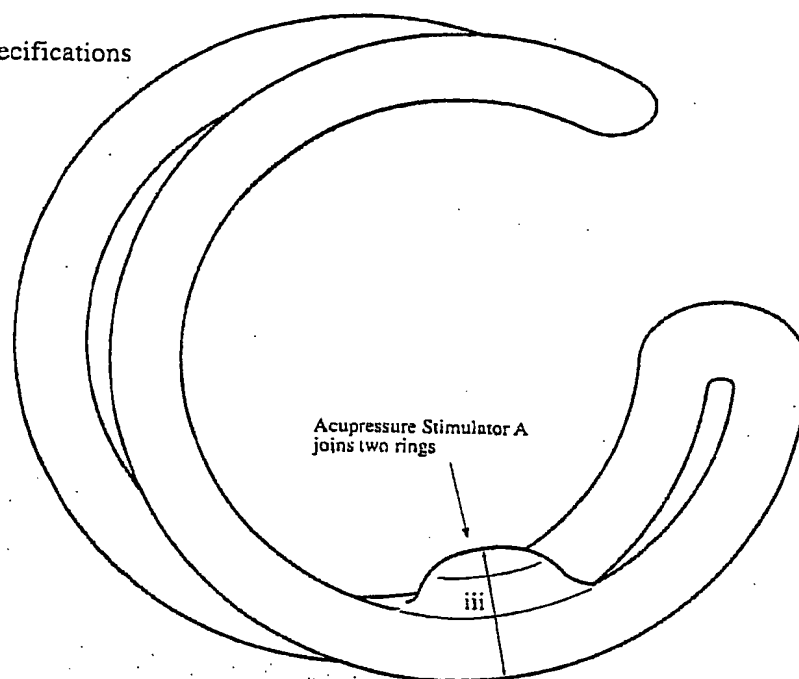


Fig. 3A

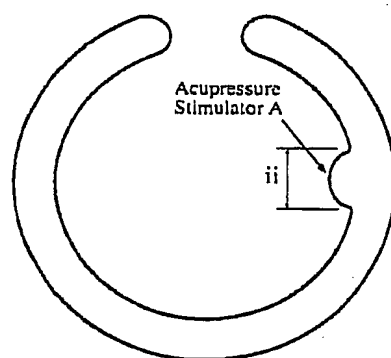


Fig. 3B

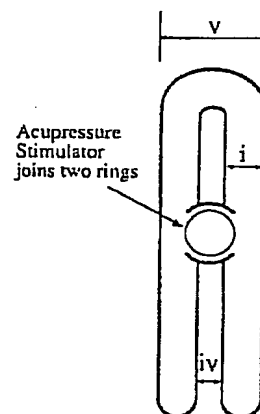


Fig. 3C

Fig 3a	min	max	optimum
iii	2.0	4.0	2.8
fig 3b			
ii	3.0	8.0	7.0
fig 3c			
i	1.4	2.0	1.56
iv	0.5	3.0	1.0
v	3.3	7.0	4.12

All measurements in millimetres

Technical specifications

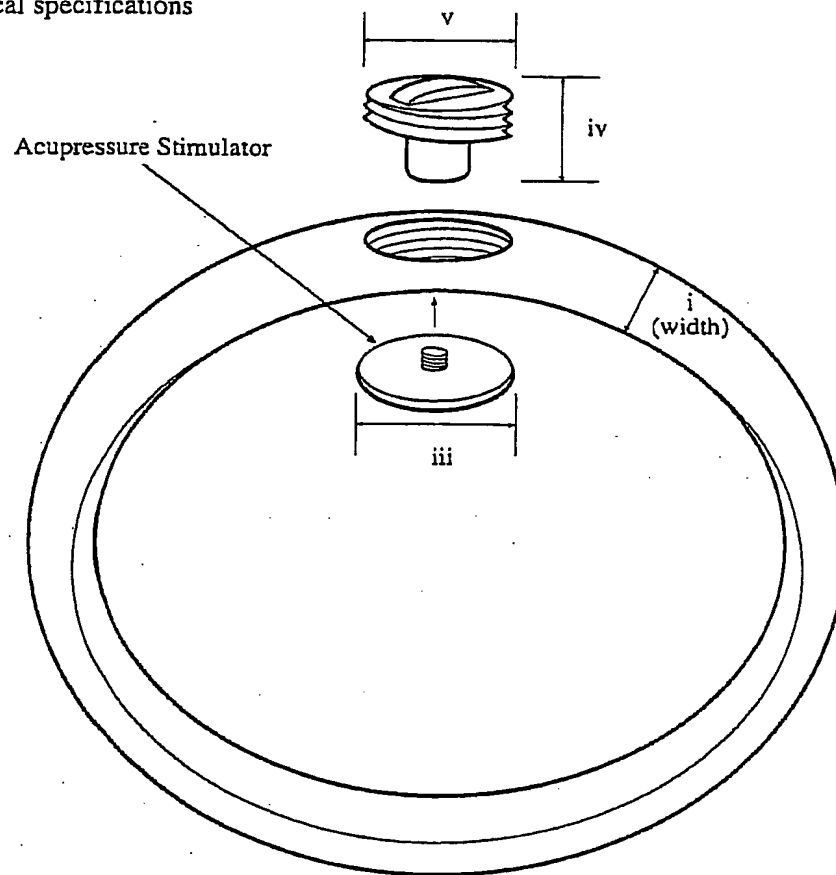


Fig. 4A

Acupressure Stimulator
assembled

Safety lock mechanism to prevent overtightening

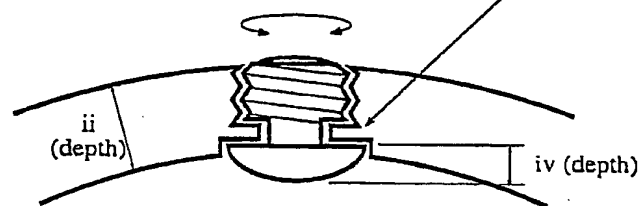


Fig. 4B

Fig 4a	min	max	optimum
i	3.0	8.0	4.0
iii	3.0	4.5	3.8
v	2.8	4.3	3.5
vi	1.0	3.5	2.0
Fig 4b			
ii	1.5	4.5	3.0
iv	1.0	2.5	1.6

All measurements in millimetres

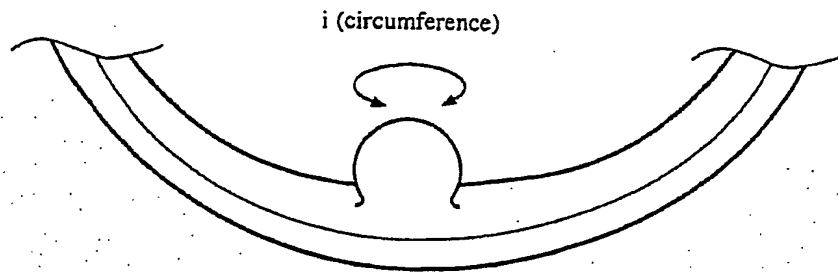


Fig. 5A

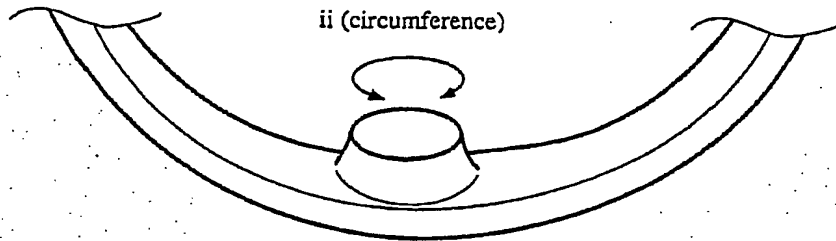


Fig. 5B

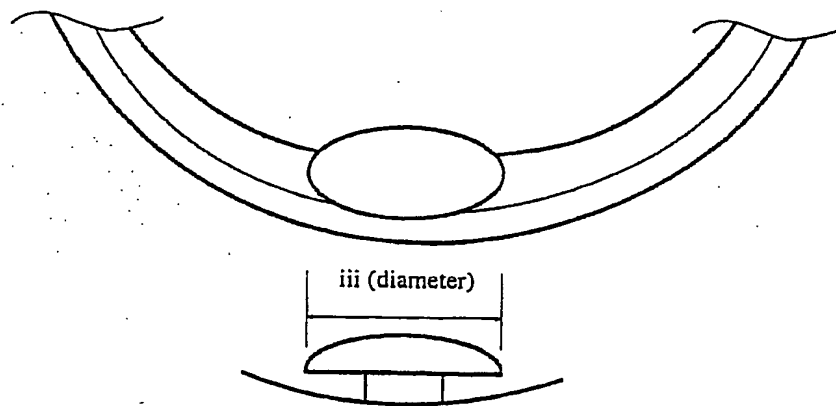


Fig. 5C

Fig 5a	min	max	optimum
i	8.2	10.8	9.7
Fig 5b			
ii	8.0	10.8	9.4
Fig 5c			
iii	4.0	9.4	8.0

All measurements in millimetres

Acupressure Meridian

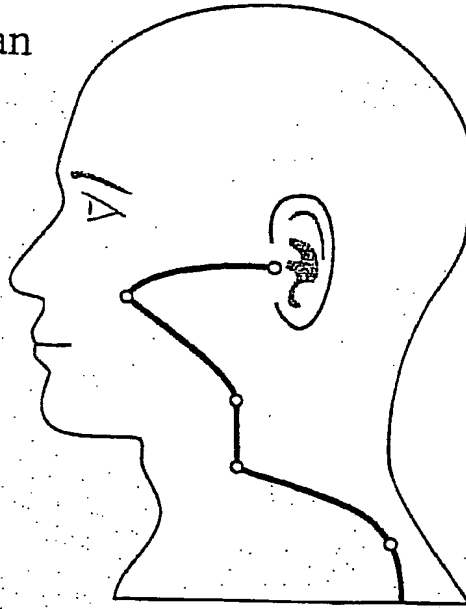


Fig. 6A

Small intestine meridian

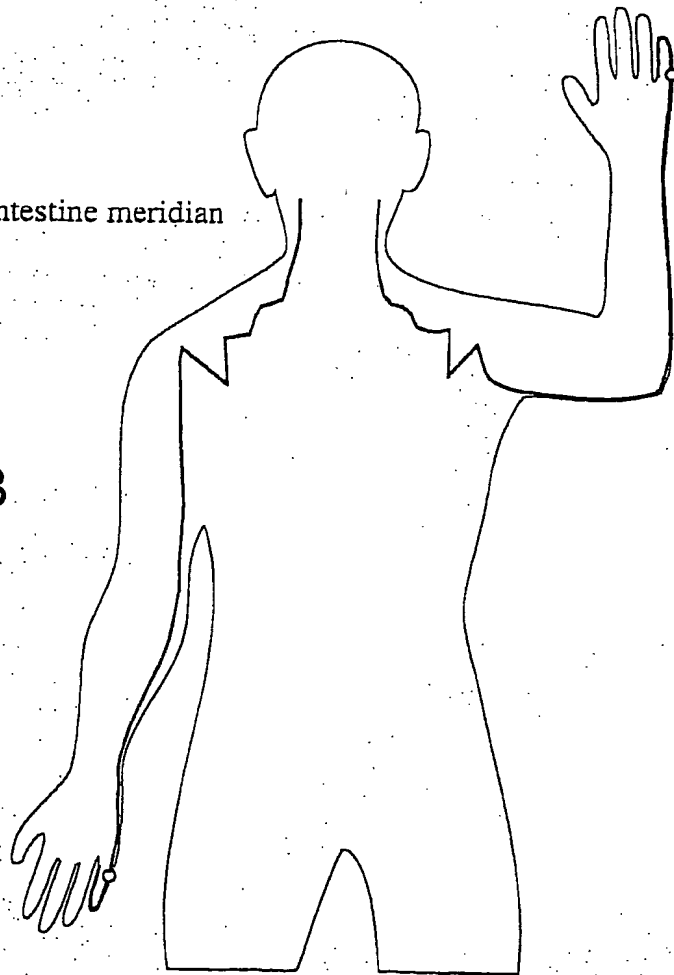


Fig. 6B

Acupressure Meridian

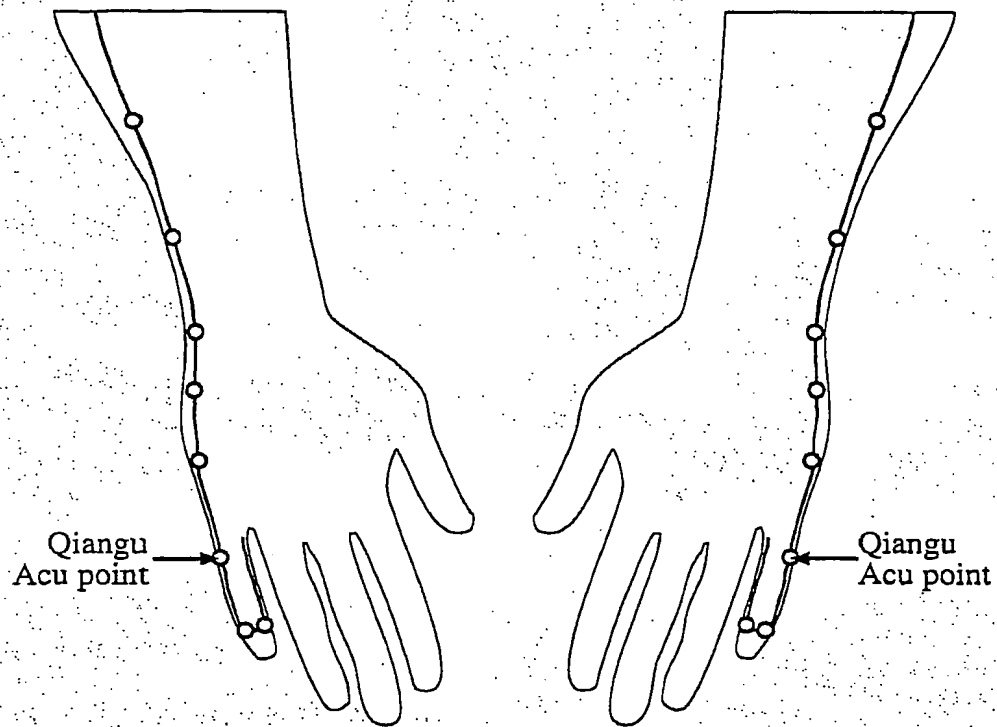


Fig. 7A

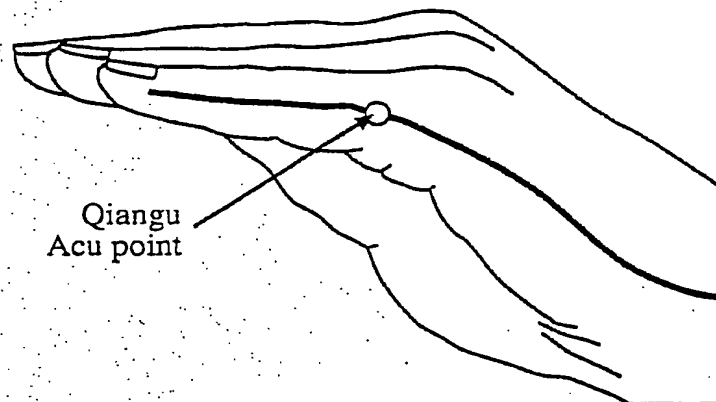


Fig. 7B



1/7

Technical specifications

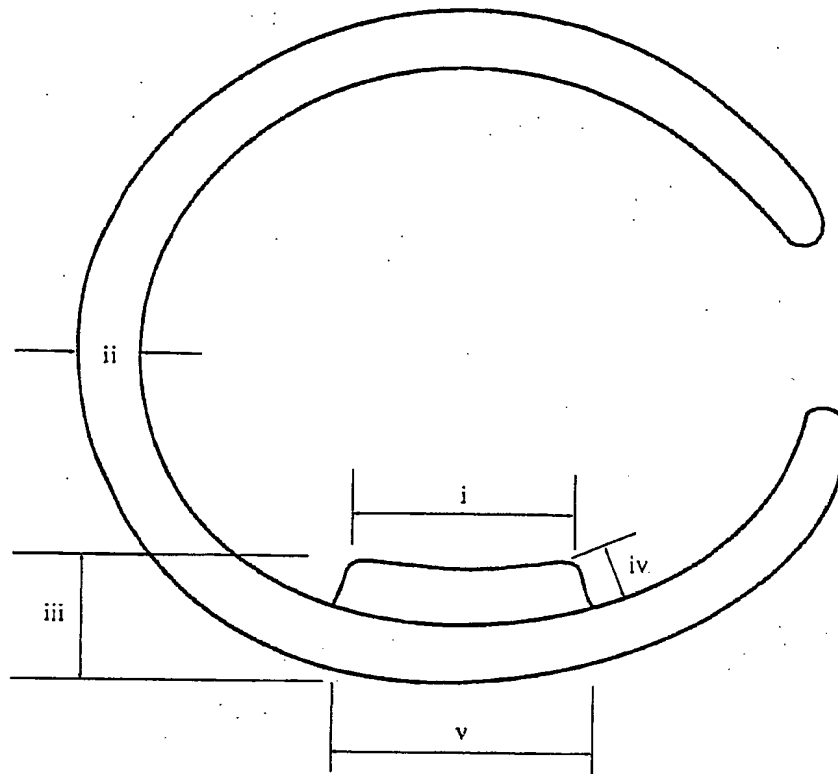


Fig. 1

Fig 1	min	max	optimum
i	6.0	10.0	8.0
ii	0.8	1.8	1.0
iii	2.0	3.8	2.8
iv	1.0	2.5	1.6
v	8.0	12.0	10.0

All measurements in millimetres

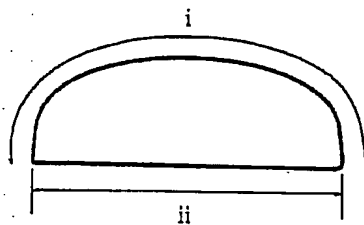


Fig. 2A

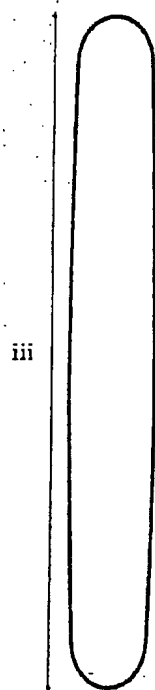


Fig. 2B

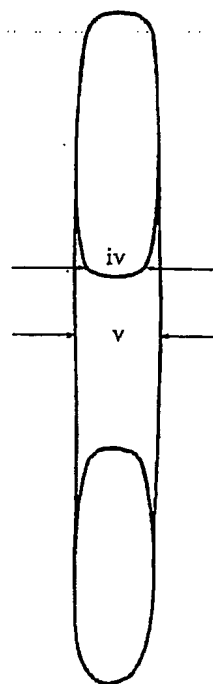


Fig. 2C

Fig 2a	min	max	optimum
i	4.9	10.0	6.5
ii	3.0	8.0	4.5
Fig 2b			
iii	18.0	26.0	22.4
Fig 2c			
iv	3.0	8.0	4.0
v	3.0	8.0	4.5

All measurements in millimetres

Technical specifications

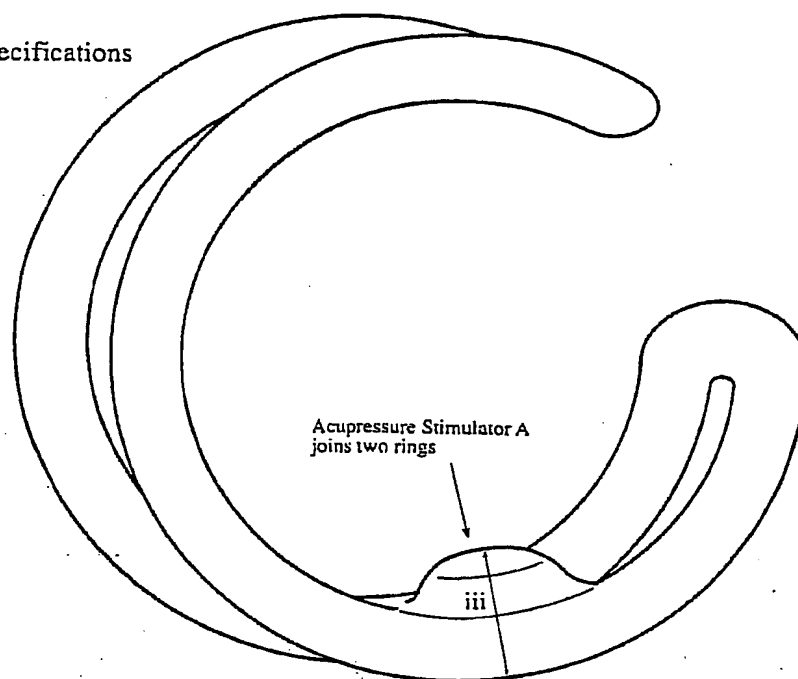


Fig. 3A

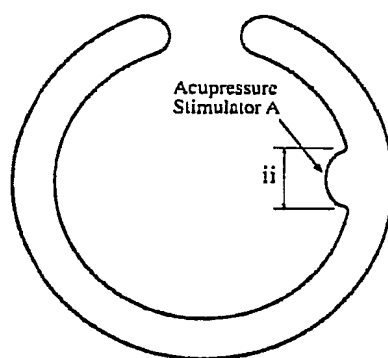


Fig. 3B

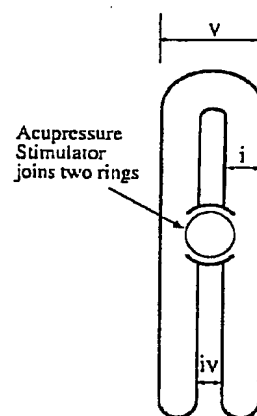


Fig. 3C

Fig 3a	min.	max	optimum
iii	2.0	4.0	2.8
fig 3b			
ii	3.0	8.0	7.0
fig 3c			
i	1.4	2.0	1.56
iv	0.5	3.0	1.0
v	3.3	7.0	4.12

All measurements in millimetres

Technical specifications

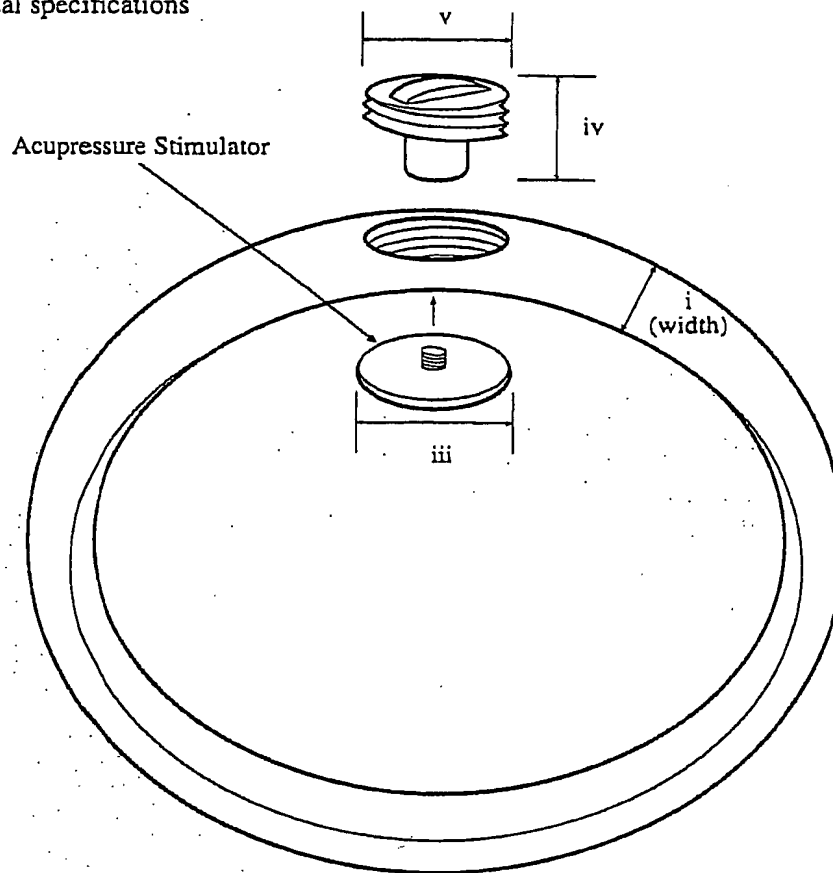


Fig. 4A

Acupressure Stimulator
assembled

Safety lock mechanism to prevent overtightening

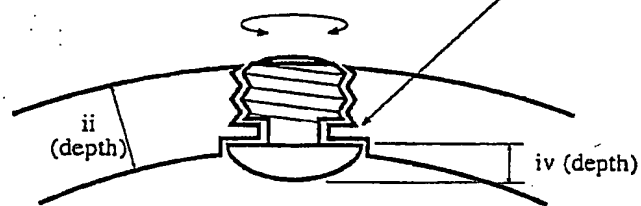


Fig. 4B

Fig 4a	min	max	optimum
i	3.0	8.0	4.0
iii	3.0	4.5	3.8
v	2.8	4.3	3.5
vi	1.0	3.5	2.0
Fig 4b			
ii	1.5	4.5	3.0
iv	1.0	2.5	1.6

All measurements in millimetres

Technical specifications

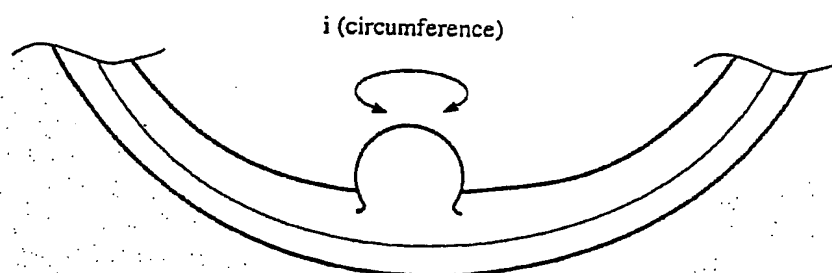


Fig. 5A

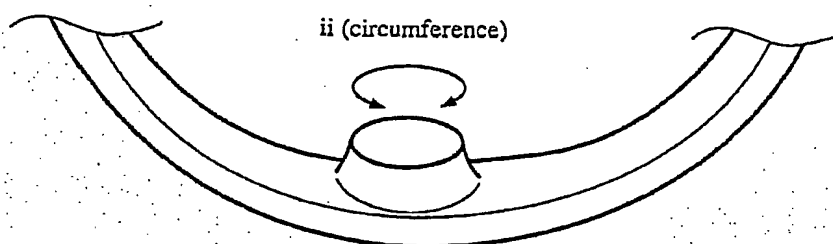


Fig. 5B

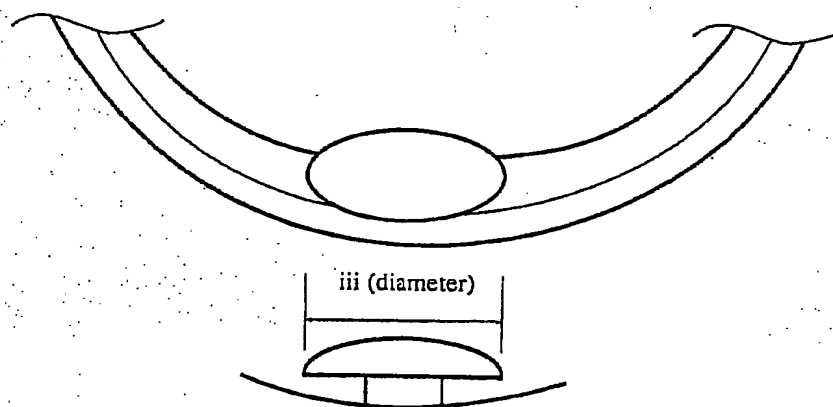



Fig. 5C

Fig 5a	min	max	optimum
i	8.2	10.8	9.7
Fig 5b			
ii	8.0	10.8	9.4
Fig 5c			
iii	4.0	9.4	8.0

All measurements in millimetres


Acupressure Meridian

Fig. 6A

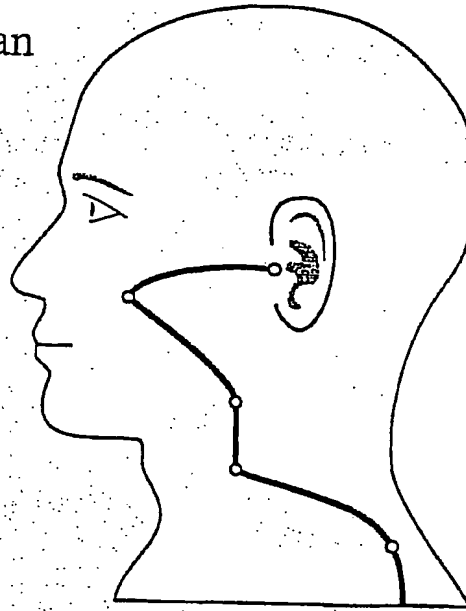

Small intestine meridian

Fig. 6B

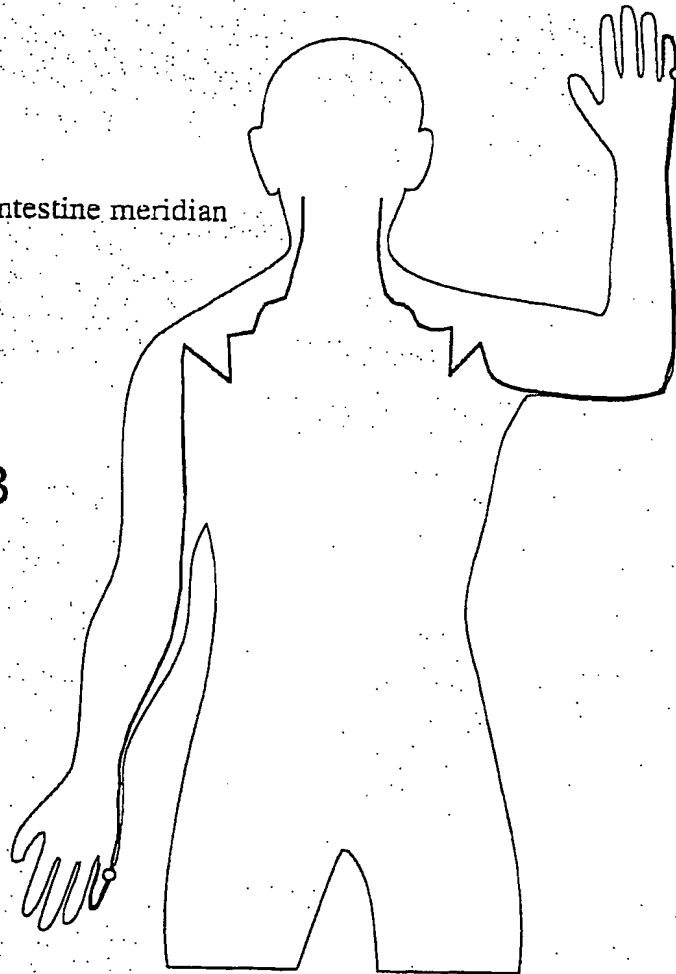

Acupressure Meridian

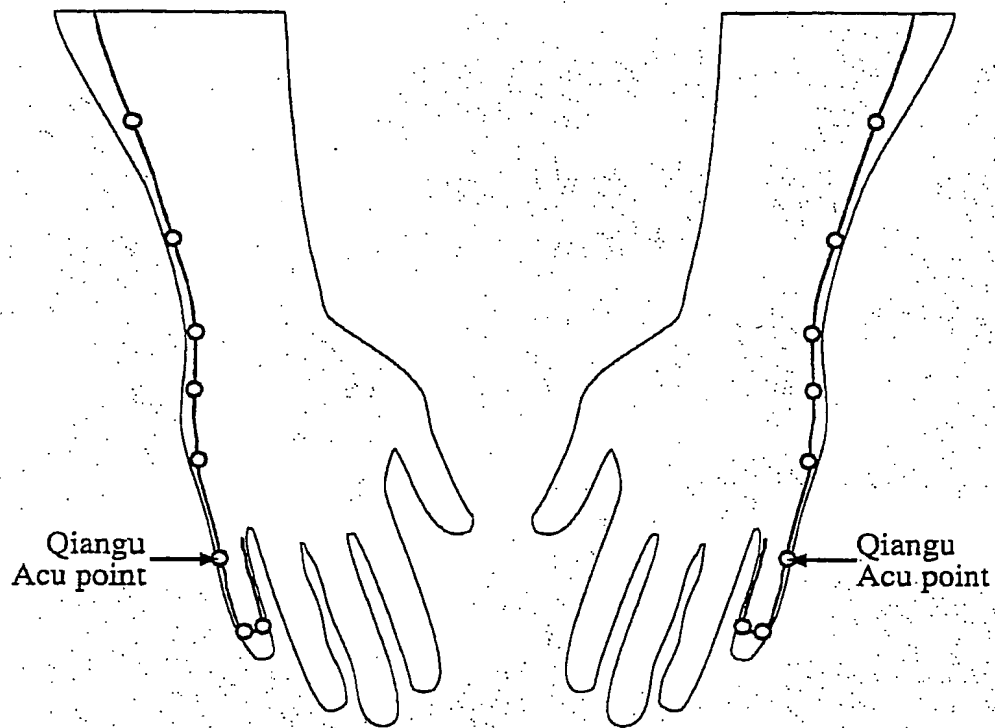


Fig. 7A

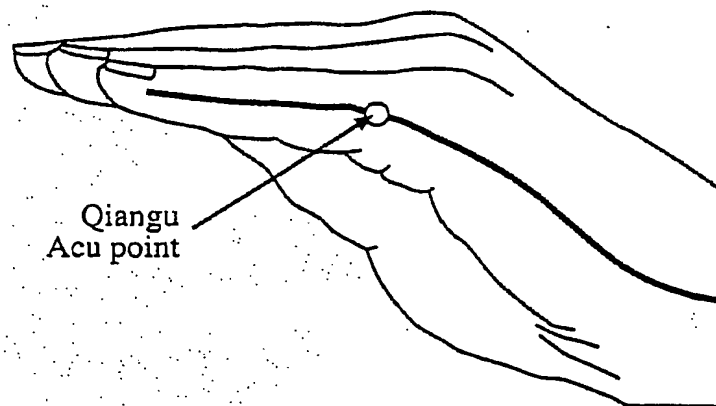


Fig. 7B